

BS EN ISO 7963:2010



BSI Standards Publication

**Non-destructive testing
— Ultrasonic testing —
Specification for calibration
block No. 2 (ISO 7963:2006)**

bsi.

...making excellence a habit.™

National foreword

This British Standard is the UK implementation of EN ISO 7963:2010. It is identical to ISO 7963:2006. It supersedes BS EN 27963:1992 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee WEE/46, Non-destructive testing.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© BSI 2010

ISBN 978 0 580 70835 0

ICS 25.160.40

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 September 2010.

Amendments issued since publication

Date	Text affected

EUROPEAN STANDARD
NORME EUROPÉENNE
EUROPÄISCHE NORM

EN ISO 7963

September 2010

ICS 25.160.40

Supersedes EN 27963:1992

English Version

Non-destructive testing - Ultrasonic testing - Specification for
calibration block No. 2 (ISO 7963:2006)

Essais non destructifs - Contrôle par ultrasons -
Spécifications relatives au bloc d'étalonnage n° 2 (ISO
7963:2006)

Zerstörungsfreie Prüfung - Ultraschallprüfung -
Beschreibung des Kalibrierkörpers Nr 2 (ISO 7963:2006)

This European Standard was approved by CEN on 26 August 2010.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

The text of ISO 7963:2006 has been prepared by Technical Committee ISO/TC 135 "Non-destructive testing" of the International Organization for Standardization (ISO) and has been taken over as EN ISO 7963:2010 by Technical Committee CEN/TC 138 "Non-destructive testing" the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by March 2011, and conflicting national standards shall be withdrawn at the latest by March 2011.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN 27963:1992.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and the United Kingdom.

Endorsement notice

The text of ISO 7963:2006 has been approved by CEN as a EN ISO 7963:2010 without any modification.

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Dimensions	1
5 Material	1
6 Preparation	3
7 Marking	3
8 Method of use	3
8.1 Setting of the time base	3
8.2 Sensitivity setting and probe checking	5
9 Certificate	7
Annex A (normative) Calibration block characteristics and use	8
Bibliography	9

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

ISO 7963 was prepared by Technical Committee ISO/TC 44, *Welding and allied processes*, Subcommittee SC 5, *Testing and inspection of welds*.

This second edition cancels and replaces the first edition (ISO 7963:1985), which has been technically revised.

Introduction

Calibration block No. 2 differs in size and shape from that described in ISO 2400.

Calibration block No. 2 is very much smaller and lighter, and its geometry is much simpler.

Calibration block No. 2 does not offer as much scope as the larger block; in particular it is not meant to check an ultrasonic flaw detector completely.

However, calibration block No. 2 makes it possible, during practical testing, to check simply, from time to time, the setting of the time base and the sensitivity of the ultrasonic equipment. Moreover, it is suited to checking the beam angle and the probe index of miniature angle-beam probes.

NOTE Calibration block No. 1 is currently specified in EN 12223.

Requests for official interpretations of any aspect of this International Standard should be directed to the Secretariat of ISO/TC 44/SC 5 via your national standards body, a complete listing which can be found at www.iso.org.

Non-destructive testing — Ultrasonic testing — Specification for calibration block No. 2

1 Scope

This International Standard specifies the dimensions, material, manufacture and methods of use for calibration block No. 2 for calibrating and checking ultrasonic testing equipment.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 4287, *Geometrical Product Specifications (GPS) — Surface texture: Profile method — Terms, definitions and surface texture parameters*

ISO 5577, *Non-destructive testing — Ultrasonic inspection — Vocabulary*

EN 10025-1, *Hot rolled products of structural steels — Part 1: General technical delivery conditions*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 5577 apply.

4 Dimensions

The dimensions of the block are given in Figure 1.

The tolerances are $\pm 0,1$ mm, except on the length of the engraved scale where it is $\pm 0,5$ mm.


Average surface roughness values, R_a , are defined in accordance with ISO 4287.

The thickness of the block can be greater than 12,5 mm (see A.1).

5 Material

The calibration block shall be made of steel of grade S355JO in accordance with EN 10025-1 or equivalent.

Dimensions in millimetres,
surface roughness in micrometres

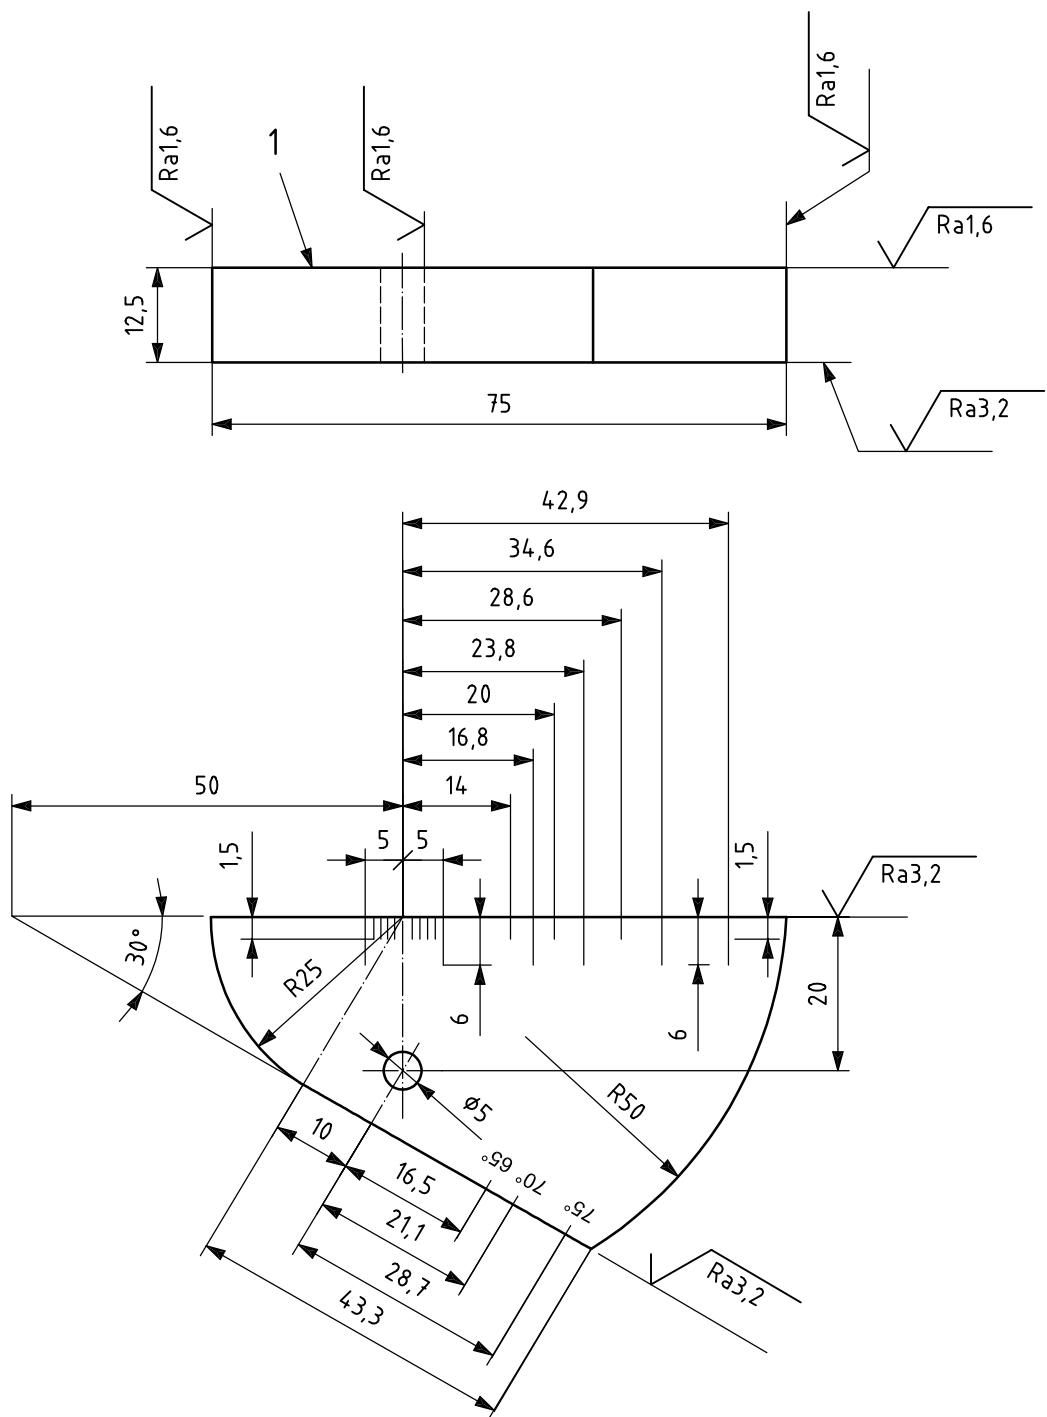

Key

1 reflection surface

Figure 1 — Calibration block No. 2 for ultrasonic testing — Dimensions of block and scales

6 Preparation

The calibration block shall be homogeneous and free from defects revealed by ultrasonic testing (see A.2).

In order to obtain a fine grain structure and good homogeneity, before final machining the block shall be heat treated as follows:

- a) maintain at 920 °C for 30 min with water-quenching;
- b) reheating to 650 °C for at least 2 h with cooling in still air.

After heat treatment, and prior to machining, the block shall undergo further ultrasonic testing from two different directions at right angles to each other and in the direction of rolling.

At least 2 mm shall be removed from all surfaces after heat treatment. All dimensions and surface finishes shall be in accordance with Figure 1.

In order to prevent parasitic effects, the depth of the marks of the engraved scale shall be $0,1 \text{ mm} \pm 0,05 \text{ mm}$. The length of the marks shall be 6 mm and the tolerance on the positioning of the marks shall be $\pm 0,2 \text{ mm}$.

On completion of machining, a final ultrasonic testing shall be carried out.

The velocity of longitudinal waves shall be verified as being $5\ 920 \text{ m/s} \pm 30 \text{ m/s}$ and the velocity of transverse waves shall be verified as being $3\ 255 \text{ m/s} \pm 15 \text{ m/s}$.

7 Marking

Reference marks on block No. 2 shall be permanently marked as shown in Figure 1.

Additionally the block shall be permanently marked with

- the manufacturer's trade mark,
- the number of this International Standard, and
- a unique serial number.

8 Method of use

8.1 Setting of the time base

To set the time base, the leading edge (left side) of successive echoes shall be adjusted to coincide with the appropriate scale markings on the screen of the measuring equipment.


The pulse-travel time depends on the velocity of ultrasonic waves in the material examined.

8.1.1 Calibration of the time base up to 250 mm with a straight beam probe


The position of the probe on the reflective side of the calibration block shall be as indicated in Figure 2a). Figure 2b) is a schematic representation of the screen (A-scan) of the instrument for calibration of a range of 50 mm.

NOTE Depending on the probe and the frequency used, difficulties can arise when calibrating distances greater than 10 times the thickness of the block.

Dimensions in millimetres

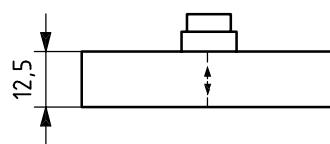

a) Position of probe on the calibration block




b) Schematic representation of the A-scan for calibration of a range of 50 mm

Figure 2 — Calibration of time base up to 250mm with a straight-beam probe


8.1.2 Calibration of the time base for 100 mm or 125 mm with a miniature angle-beam probe

The position of the miniature shear-wave probe on the calibration block shall be as shown in Figure 3a) for a distance of 125 mm and in Figure 3b) for a distance of 100 mm. The screen of the instrument for the calibration of these two ranges is shown schematically in Figures 3a) and 3b).

Dimensions in millimetres

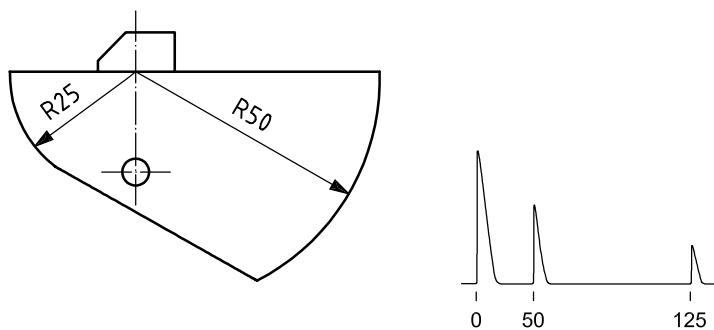

a) For a range of 125 mm

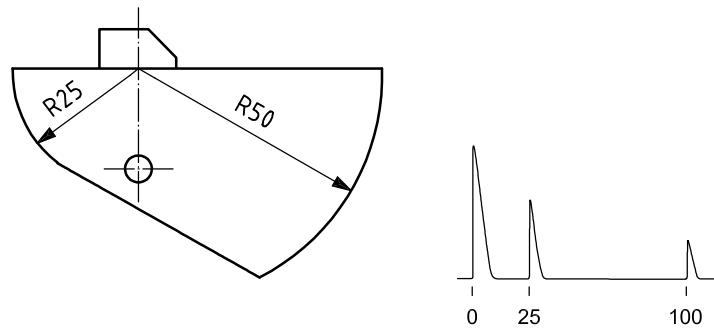

b) For a range of 100 mm

Figure 3 — Position of miniature shear-wave probe on the calibration block

8.2 Sensitivity setting and probe checking

8.2.1 General

A large number of factors can influence the sensitivity setting (see A.3).

8.2.2 Longitudinal-wave probes — Sensitivity setting

The probe shall be placed in position "a" as indicated in Figure 4.

The A-scan representing the successive echoes shall be used as a reference for setting sensitivity.

The reflection from the 5 mm diameter hole, position "b" in Figure 4 may also be used, the probe being placed so that the corresponding echo amplitude is at its maximum.

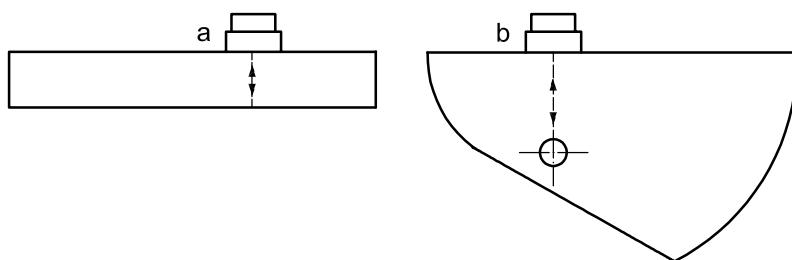


Figure 4 — Straight-beam probes — Sensitivity setting

8.2.3 Miniature shear-wave probes

8.2.3.1 Sensitivity setting

The maximum echo from the 5 mm diameter hole shall be used as a reference for setting sensitivity (see Figure 5, position "a").

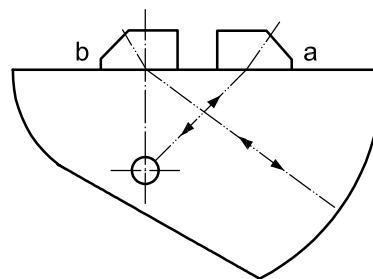


Figure 5 — Miniature angle-beam probes — Sensitivity setting

Alternatively, it is possible to make use of the reflections from the cylindrical surfaces of radii 50 mm and 25 mm, respectively.

In this case, there are two possibilities:

- by using a calibrated gain control, the amplitude of the echo from the cylindrical surface is initially set to 80 % of screen height and subsequently adjusted to the level desired (see Figure 5, position "b");
- without the use of a calibrated gain control, the successive echoes from the cylindrical surfaces can be used for the adjustment of sensitivity (see Figure 6).

When checking probes, the acoustic coupling is an important factor, and when comparing probes, the same coupling medium shall be used.

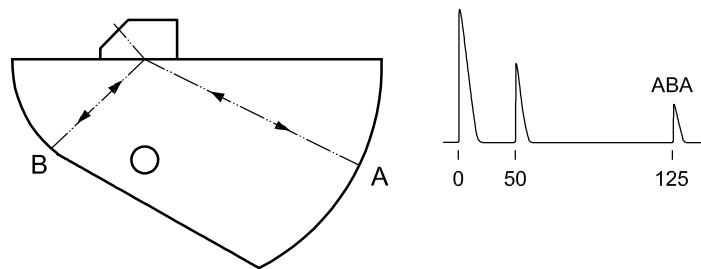


Figure 6 — Miniature angle-beam probes — Sensitivity setting without calibrated gain control

8.2.3.2 Determination of the position of the probe index

The miniature angle-beam probe shall be positioned as shown in Figures 3a) or 3b) and moved parallel to the main faces of the calibration block until the amplitude of the echo from the cylindrical surface has reached its maximum.

The probe index coincides with the centre mark of the millimetre scale of the block.

8.2.3.3 Determination of beam angle

The echo obtained from the 5 mm diameter hole is used to determine the beam angle.

The miniature shear-wave probe shall be moved parallel along the main faces of the calibration block until the amplitude of the echo from the 5 mm diameter hole has reached its maximum.

The beam angle is obtained either by direct reading of the scale engraved on the calibration block, coinciding with the index mark of the probe, or by interpolation if the position found does not coincide with one of the scale lines.

The positions shown in Figure 7 make it possible to check beam angles of 45°, 60° and 70° probes.

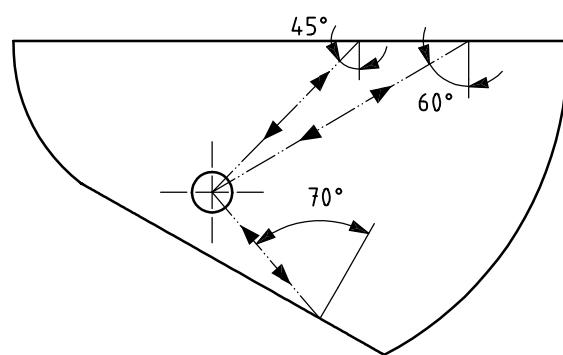


Figure 7 — Miniature angle-beam probes — Determination of beam angle

9 Certificate

For each block, a certificate shall be issued by the manufacturer stating:

- a) that the block complies with this International Standard (ISO 7963);
- b) the mean value of the measured longitudinal wave velocities, v_l ;
- c) the mean value of the measured transverse wave velocities, v_t .

Annex A (normative)

Calibration block characteristics and use

A.1 Thickness of the block for calibration of “non-miniature” probes

A thicker block may be used, for example 20 mm or 25 mm thick, when using non-miniature probes.

A.2 Ultrasonic inspection of material before and after final machining

Two inspections with a longitudinal-wave probe (transducer diameter 10 mm; frequency 6 MHz) are recommended:

- a) with the probe positioned as shown in Figure 2a), the amplitude of the fourth back echo shall be greater than the noise level produced by the grain structure when the latter is increased by at least 50 dB;
- b) no echo arising from any defect in the homogeneity of the material shall have an amplitude greater than the grain scatter noise level.

A.3 Factors to be taken into consideration for the setting of sensitivity

The following factors, divided into four main groups, should be taken into account when setting the sensitivity:

- a) equipment: pulse energy, frequency, pulse shape, amplification, etc.;
- b) probe used: type, size, acoustic impedance, transducer damping, polar diagram, etc.;
- c) material to be examined: surface condition (in connection with coupling), kind of material (its absorption), etc.;
- d) defect analysis: shape, orientation, nature, etc.

Bibliography

- [1] ISO 2400, *Welds in steel — Reference block for the calibration of equipment for ultrasonic examination*
- [2] EN 12223, *Non-destructive testing — Ultrasonic examination — Specification for calibration block No.1*

This page deliberately left blank

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.TM